



Programming Maintenance Fluids in Guardrails


1. Select Channel to infuse Maintenance Fluids.
2. Select “Guardrails IV Fluids”

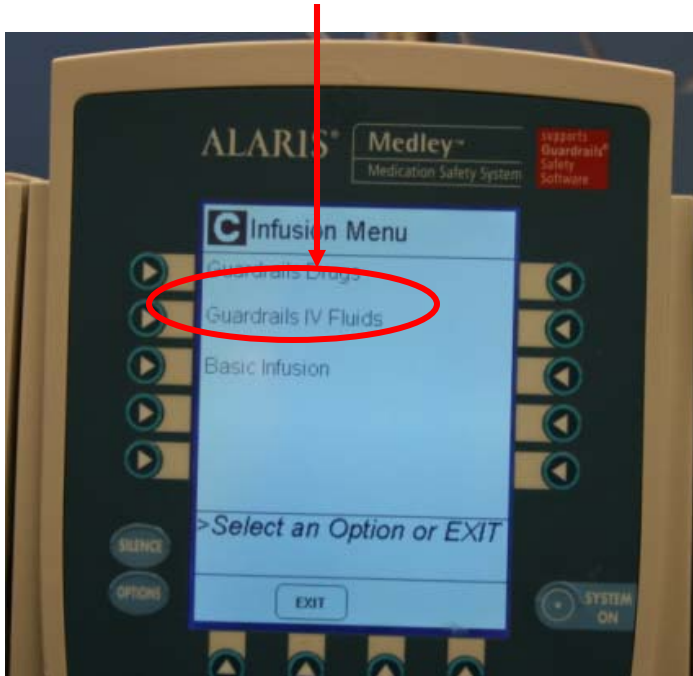


3. Select Patient Weight range (may need to page down to find patient weight range)

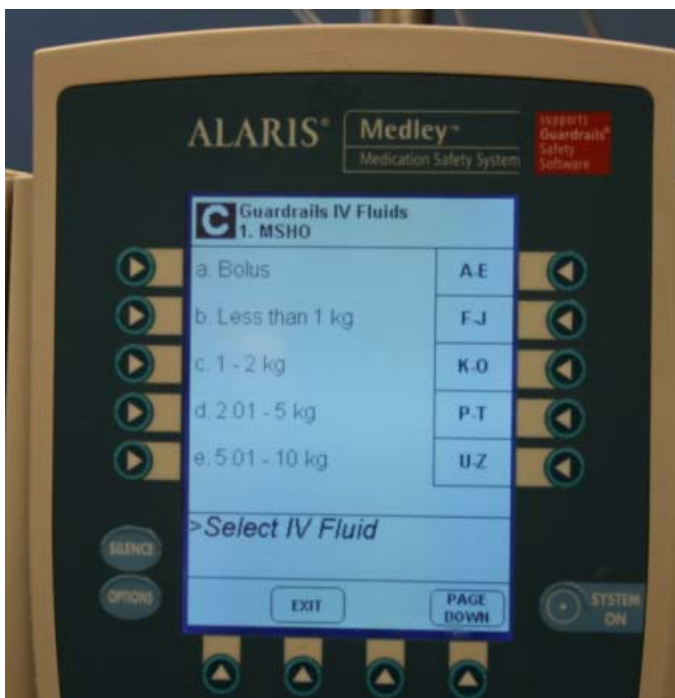

4. Confirm patient weight range

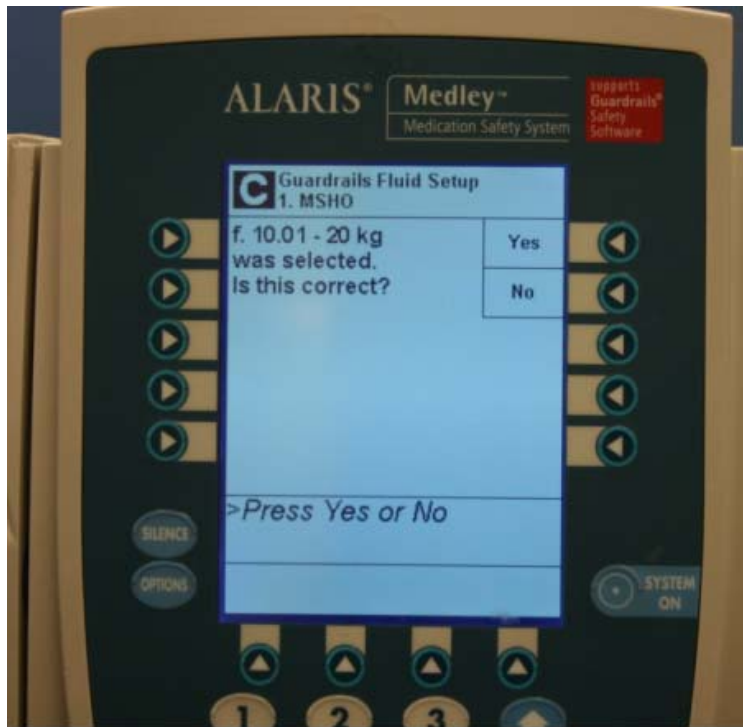

5. Enter Rate and Volume to be infused

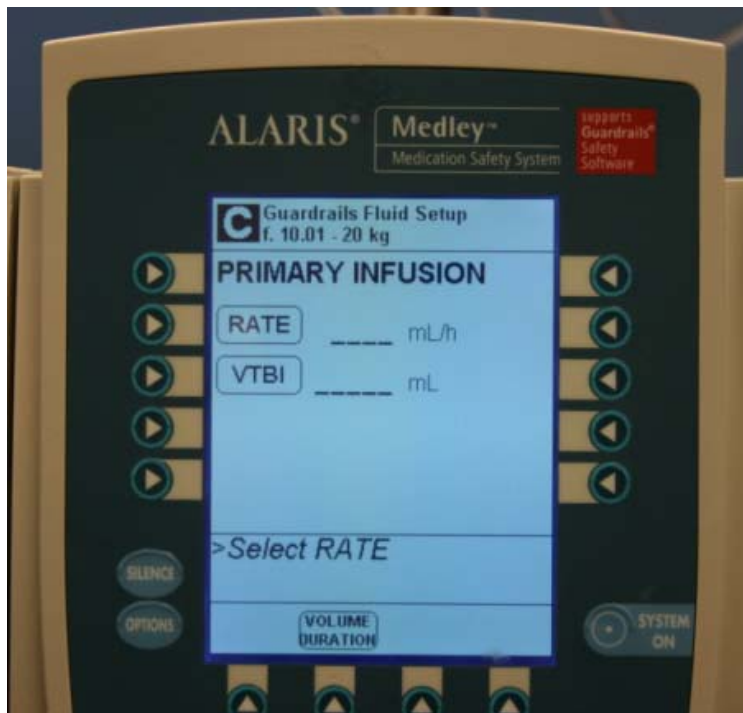

6. Confirm Rate and Volume; Select "Start"